


Power-off procedure for a spectrometer



Overview

Aspirate distilled water for at least 5 minutes (flame analysis only). Turn off the instrument and disconnect the spectrometer from mains power. Shut off all gas supplies at the regulators/isolation valves and gas cylinders. This section describes how to shut down the system for a maintenance or service procedure. Power is removed abruptly when you place the main power circuit breaker switch in the Off (O) position. Once. How to safely vent and turn off your Agilent Single or Triple Quadrupole LC/MS system. Start up a QToF from complete shutdown. Make sure the. Stop the mass spectrometer first to confirm that the liquid phase flow rate has stopped, then standby the mass spectrometer, wait for the desolvation gas temperature to drop 100 °C below to turn off the nitrogen, clean the ion source and the inner cavity of the ion source.

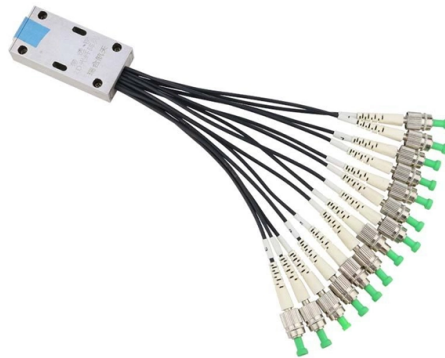

Article Content

Spectrophotometer Troubleshooting Guide

Spectrophotometer Troubleshooting Guide In a basic biology lab class, a spectrophotometer appears pretty robust and easy to use. That's still the

Sage Journals: Your gateway to world-class journal research

Hier sollte eine Beschreibung angezeigt werden, diese Seite lässt dies jedoch nicht zu.

Basic Experiment Setup and Basic NMR Spectrometer Operation

Basic Experiment Setup and Basic NMR Spectrometer Operation Setup for Bruker 300 MHz, 400 MHz, and 600 MHz NMR spectrometers:

Venting and Shutting Down your Single or Triple Quadrupole LC/MS

Spray chamber voltages, the drying gas heater, the nebulization gas flow, the detector, and other specific lens voltages are all turned off. The drying gas flow is set to standby.

Maintenance and Preventative Care for FTIR Spectrometers in Drug ...

Purpose and Scope Drug checking in community can occur in environments that are less than ideal for FTIR spectrometers (FTIRs). Infrared spectrometers are delicate instruments that require careful

How do I power-off or shut down a QDa detector that has been

OBJECTIVE: Power-off or shut down a QDa detector. PROCEDURE: Stop the mobile phase system flow to the QDa detector. Take the detector out of Operate mode and put it into Standby mode using

UV-VIS Spectrophotometer Troubleshooting and FAQs

What is the Z dimension or beam height of your Spectrometers? The power LED indicator light on my UV-VIS or Fluorescence/UV-VIS Spectrometer is red. Software Issues: Why is

Long Term Shut Down and Start Up Instructions

Shut down any accessories according to the instructions in their user guides. Aspirate distilled water for at least 5 minutes (flame analysis only). Turn off the instrument and disconnect the spectrometer

Standard operating procedure for operating JEOL EPR spectrometer

ESR Instrument : JEOL Japan Qband/X Band ESR Spectrometer Model - JES FA-200E
Accessories used : OD ESR tubes

Shut down the system

In the Tune window, click the System Off button () to put the instrument in Off condition. All high voltages are shut off, as are the sheath and auxiliary gas. Put the main power circuit breaker switch of the

How to properly startup and shutdown your Shimadzu

Shut down: If the instrument (UV-Vis, FTIR and Fluorescence) is not going to be used for an extended period, please, close the software and turn off the power

Standard Operating Procedure (SOP)

Standard Operating Procedure (SOP) This Standard Operating Procedure (SOP) describes basic chemical safety information for Mass Spectrometry (MS). Prior to conducting work with a mass

Venting and Shutting Down your Single or Triple Quadrupole LC/MS

This process normally takes less than 10 mins and the rough vacuum readings can be monitored via MassHunter or OpenLab CDS ChemStation. To shut down the Instrument Turn off the MS using the

FTIR-Operation and Calibration SOP

Standard Operating Procedure (SOP) for Operation, Calibration, Cleaning, and Maintenance of FTIR (Fourier Transform Infrared Spectrometer).

How to start up or pump down a powered down mass spectrometer

Start up a QToF from complete shutdown. Power-on the host PC and then log into Windows. Power-on the LC and let it initialize. If this instrument is an H-class/I-class/M-Class, power on the sample

Fourier Infrared Spectroscopy

Fourier Transform Infrared Spectroscopy (FTIR) is an important technique that provides an easy way to identify the presence of certain functional groups in an organic molecule. Functional groups have

Q-EXACTIVE MASS SPECTROMETER EMERGENCY PROCEDURES

Place the main power circuit breaker switch, located on the power panel on the left side panel of the mass spectrometer, in the OFF position. This turns off all power to the mass

Standard operating procedure for operating JEOL EPR spectrometer

Spectrometer is shut down while leaving in the evening. Click "shut down". Then click "power of" option. Power supply to magnet goes of bringing the value to default seting. Then the spectrometer unit

How to Use a Spectrometer: A Step-by-Step Guide

A spectrometer is an analytical tool used across various scientific disciplines to measure how a substance interacts with light. Specifically, a UV-Visible Spectrometer measures the

How To Use A Spectrophotometer

A spectrophotometer is a device used to measure light at a specific wavelength. It consists of two parts: a spectrometer and a photometer. The

Major liquid mass spectrometers on/off procedure_

After the mass spectrometer has been powered on for 10 minutes, open the MassLynx software and evacuate overnight until the next day. After full filling of the liquid phase, rinse with methanol at a flow

A Complete Guide to Shutting Down Analytical Instruments

Our guide is tailored to assist analytical chemists in identifying and fixing common LC/MS problems. Inside, you'll find guidance on solvent selection,

Procedure For Acquiring 1 (One) Spectrometer For Vis-Nir

Procedure For Acquiring 1 (One) Spectrometer For Vis-Nir Reflectances, Within The Scope Of The Financing Contract Signed With The Foundation For Science And Technology, I.P. (Fct), Under The

Standard Operating Procedure Ultraviolet Visible (UV-Vis) Spectroscopy ...

Description of Process The ultraviolet-visible spectroscopy (UV-Vis) utilizes light to determine the absorbance or transmission of a chemical species in either solid or aqueous state.

Q-EXACTIVE MASS SPECTROMETER EMERGENCY PROCEDURES

Q-EXACTIVE MASS SPECTROMETER EMERGENCY PROCEDURES If you need to turn off the mass spectrometer in an emergency, the user should do the following:

How to Operate a Spectrophotometer | HunterLab

Spectrophotometric solutions simplify the science of quantifying chromatic data for many industries. Manufacturers using a spectrophotometer

Spectrometer

A spectrometer is typically used to measure wavelengths of electromagnetic radiation (light) that has interacted with a sample. Incident light can be reflected

Shimadzu Instrument Startup and Shutdown Procedures

Molecular Spectroscopy Start up: To start up your instrument, power it on using the power switch/button on the instrument, and then open the operating software.

Agilent AA Spectrometer Shutdown Guide

1 Shut down any accessories according to the instructions in their user guides. 2 Aspirate distilled water for at least 5 minutes (flame analysis only). 3 Turn off the

Contact Us

For more information, pricing, or custom solutions, please contact us:

Website: <https://www.charratcommunication.fr>

Email: sales@charratcommunication.fr

Phone: +33 1 42 68 93 17

Address: 15 Rue de la Paix, 75002 Paris, France

This document is for informational purposes only. Specifications subject to change without notice.

